

Certificate of Analysis Data Summary

Substantive test data from the original laboratory certificate reproduced on page 2.

REGENIX QUALITY REVIEW

Original certificate follows unchanged


SAMPLE SUMMARY				CERTIFICATE REFERENCE	
PRODUCT	GLP3: RETA 10mg	PURITY	99.01%	ACCESSION #	2605270481
IDENTITY	Confirmed	NET CONTENT	10.47 mg	SEARCH CODE	Pept2605270481
APPEARANCE	White Lyophilized Powder			RECEIVED	05/27/2026
				REPORTED	05/29/2026
				LOT	RET750

ANALYTICAL RESULTS

Identity (LC-MS)	GLP RT
Purity (HPLC-UV)	99.01%
Net Content	10.47 mg

METHOD

HPLC with UV detection coupled with mass spectrometry (LC-MS).

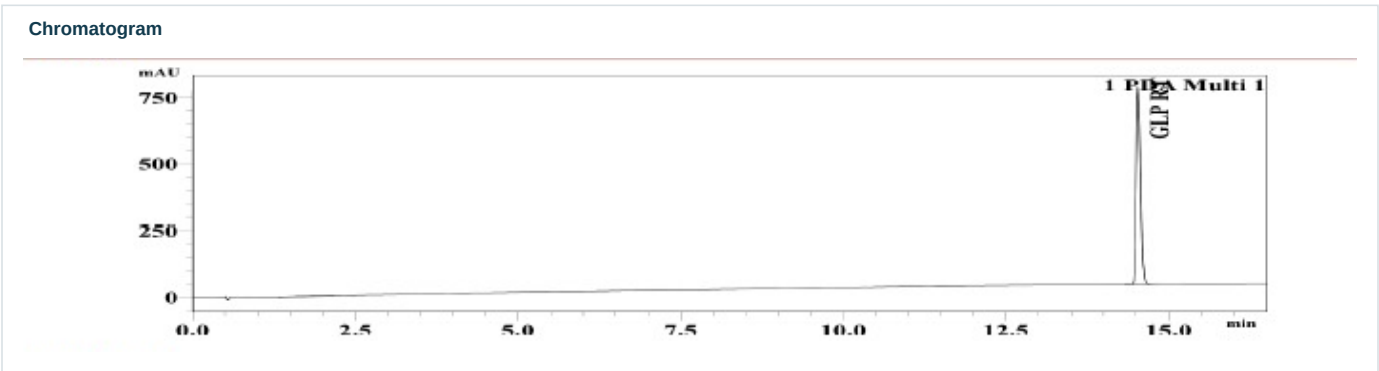

Research-use context: Analysis was conducted under standard laboratory conditions and is specific to the sample provided. Results are informational, not approved for human or veterinary use, diagnosis, therapy, or clinical application, and should be interpreted by qualified professionals. Sample integrity, handling, and experimental variables may affect accuracy and reliability.



Certificate of Analysis

FreedomDiagnosticsTesting.com

Admin@FreedomDiagnostics.net

Client:	Peptide Maxxing
Accession #:	2605270481
Search Code:	Pept2605270481
Received:	05/27/2026
Reported:	05/29/2026
Lot:	RET750

Sample Summary


Product:	GLP3: RETA 10mg	Purity:	99.01%
Identity:	Confirmed	Net Content:	10.47 mg
Appearance:	White Lyophilized Powder		

Analytical Results


Test	Result
Identity (LC-MS)	GLP RT
Purity (HPLC-UV)	99.01%
Net Content	10.47 mg

Method: HPLC with UV detection coupled with mass spectrometry (LC-MS).

Chromatogram

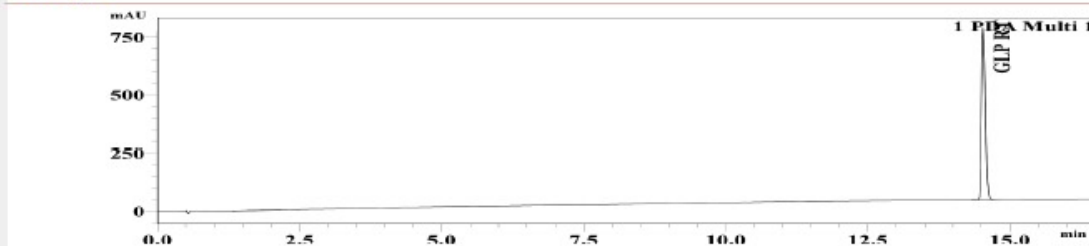

Mass Confirmation

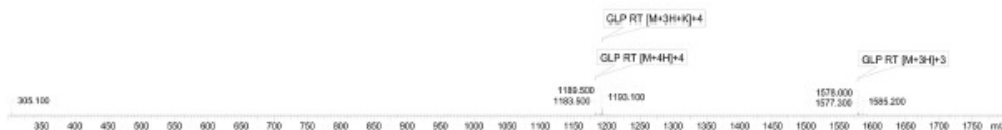

Alex Johnson

Principal Chemist

FreedomDiagnosticsTesting.com
Admin@FreedomDiagnostics.net
Proudly Owned and Operated in the USA



The peptide purity analysis reported here was conducted using LC/MS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.